

NOTHING
IS SIMPLE
IN ONCOLOGY.
**NOTHING
BUT
THIS.**



Idylla™ A revolutionary,
fully automated system that makes
molecular testing convenient and fast.
Suitable for any lab.


biocartis.com/us



“

WE AIM
TO PROVIDE
**RAPID
ACCESS**
TO HIGH-LEVEL
MOLECULAR TESTING
ANYTIME,
ANYWHERE.

THE IDYLLA™ SOLUTION - MOLECULAR TESTING SUITABLE FOR VIRTUALLY ANY LAB.

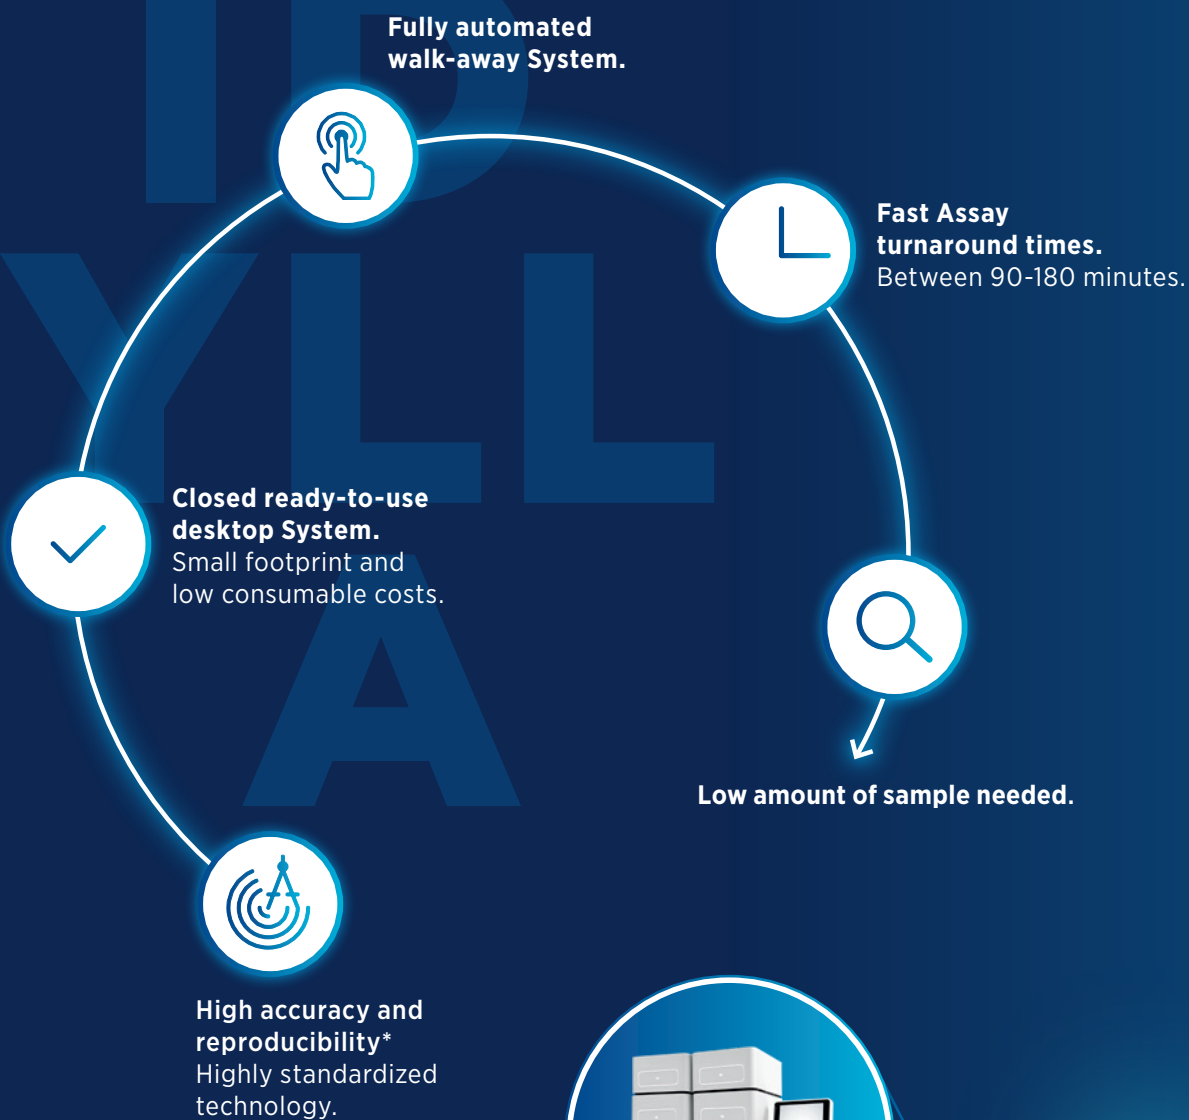

THE IDYLLA™ SYSTEM. BUILT FOR YOUR NEEDS.

Idylla™ is a modular instrument ready to accommodate your lab's throughput even as it changes over the years.



*For Idylla™ IVD Tests.

IDYLLA™ FITS ANY SIZE LAB



IDYLLA™ IS A COST-EFFECTIVE IN-HOUSE SOLUTION EVEN FOR SMALL SAMPLE VOLUMES

- Easy to implement and maintain
- No molecular infrastructure needed
- No batching needed




IDYLLA™ PROVIDES AN ULTRA-RAPID ACTIONABLE SOLUTION COMPLEMENTING COMPREHENSIVE NGS PROGRAMS

- Short turnaround time and minimal hands-on time
- Minimal sample input requirements
- On-demand testing
- Seamless integration into virtually any laboratory workflow




THE REVOLUTIONARY IDYLLA™ WORKFLOW

STANDARD SOLID BIOPSY WORKFLOW

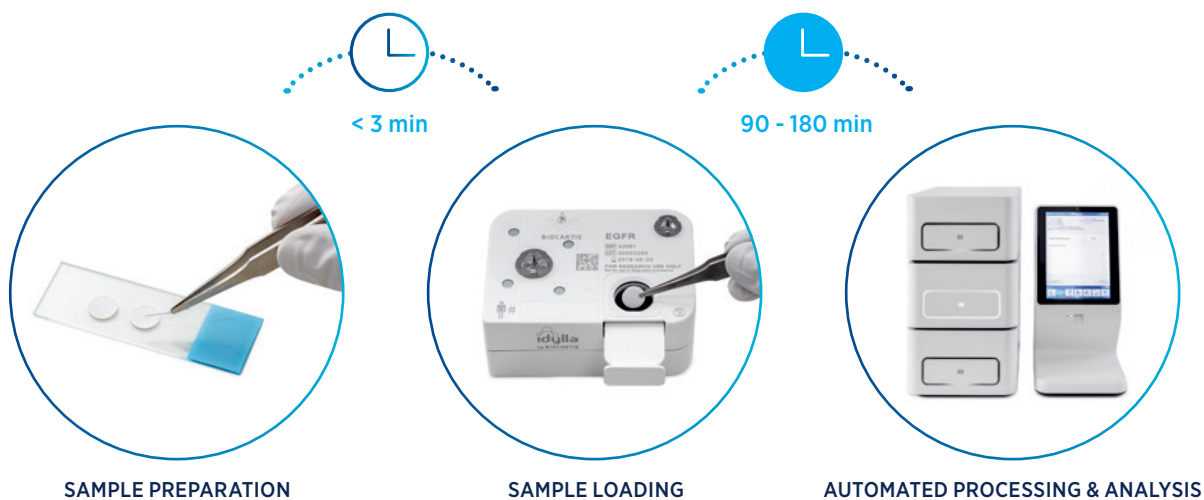

LIQUID BIOPSY WORKFLOW

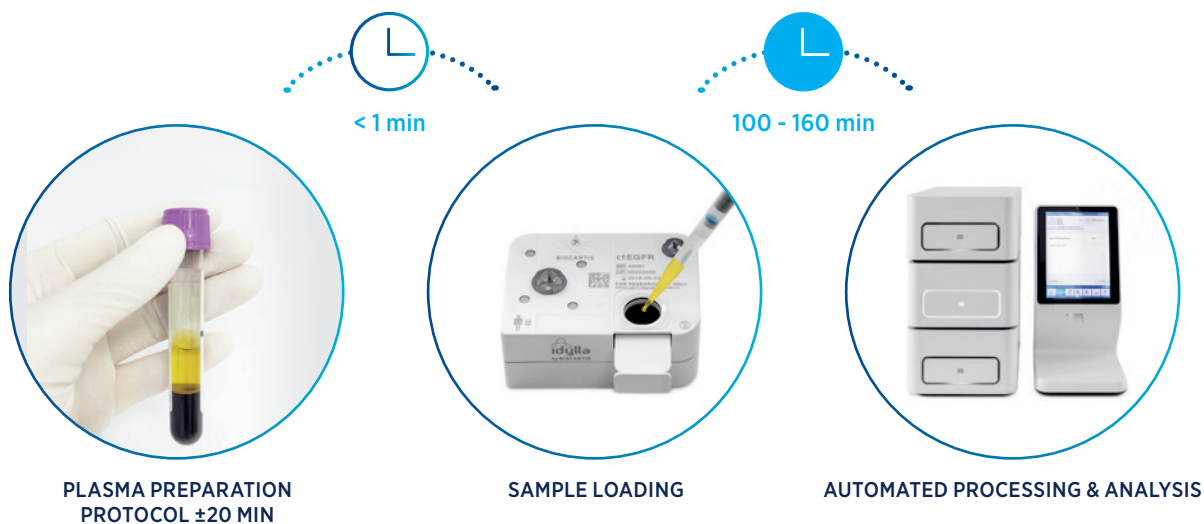

IDYLLA™ COMPARED TO OTHER TECHNOLOGIES

MINIMAL HANDS-ON AND ASSAY TURNAROUND TIMES



REDUCED NUMBER OF INSTRUMENTS AND CONSUMABLES NEEDED

	OTHER RT-PCR	NEXT GENERATION SEQUENCING
INSTRUMENTS		
CONSUMABLES		
LAB INFRASTRUCTURE (# OF ROOMS)	3	4

Based on workflow exercise in real-life laboratory setting. Reference technologies used: Illumina MiSeq® and Qiagen Therascreen®.

THE IDYLLA™ ASSAYS. MINIMAL SAMPLE REQUIREMENTS AND VERSATILE SAMPLE TYPES.



SOLID BIOPSY SPECIMEN REQUIREMENTS

IVD TESTS

MSI (510(k))	• 1 x 4 µm FFPE tissue section	→ 62.5-750 mm ²
	• 1 x 5 µm FFPE tissue section	→ 50-600 mm ²
	• 1 x 10 µm FFPE tissue section	→ 25-300 mm ²
	• Neoplastic cells ≥ 33% - if less, macrodissection is required	

MSI-CDx (PMA)	• 1 x 4 µm FFPE tissue section	→ 62.5-750 mm ²
	• 1 x 5 µm FFPE tissue section	→ 50-600 mm ²
	• 1 x 10 µm FFPE tissue section	→ 25-300 mm ²
	• Neoplastic cells ≥ 33% - if less, macrodissection is required	

RUO ASSAYS

EGFR	• 1 x 5 µm FFPE tissue section	→ ≥ 1 mm ²
	• Neoplastic cells ≥ 10% - if less, macrodissection is required	

GeneFusion	• 1 x 5 µm FFPE tissue section	→ 20-100 mm ²
	• 3 x 5 µm FFPE tissue sections	→ < 20 mm ²
	• Neoplastic cells ≥ 10% - if less, macrodissection is required	

BRAF	• 1 x 5 µm FFPE tissue section	→ 50-600 mm ²
	• 1 x 10 µm FFPE tissue section	→ 25-300 mm ²
	• Neoplastic cells ≥ 50% - if less, macrodissection is required	

KRAS, NRAS-BRAF-EGFR S492R	• 1 x 5 µm FFPE tissue section	→ 50-600 mm ²
	• 1 x 10 µm FFPE tissue section	→ 25-300 mm ²
	• Neoplastic cells ≥ 10% - if less, macrodissection is required	

POLE-POLD1	• 1 x 5 µm FFPE tissue section	→ 50-600 mm ²
	• 1 x 10 µm FFPE tissue section	→ 25-300 mm ²
	• Neoplastic cells ≥ 10% - if less, macrodissection is required	

IDH1-2	• 50 µl extracted DNA (concentration ≥ 10 ng/µl)	
	• 10 µl blood or bone marrow	
	• Maximum 3 FFPE tissue sections	
	• Neoplastic cells ≥ 10% - if less, macrodissection is required	

PIK3CA-AKT1	• 1 x 5 µm FFPE tissue section	→ 50-600 mm ²
	• 1 x 10 µm FFPE tissue section	→ 25-300 mm ²
	• Neoplastic cells ≥ 20% - if less, macrodissection is required	



LIQUID BIOPSY SPECIMEN REQUIREMENTS

RUO ASSAYS

- 1 or 2 ml plasma (depending on Assay) and two validated tube types:



K²EDTA tubes

process within 4 hours



Streck Cell-Free DNA BCT® Tubes

process within 3 days

- Used in the following Idylla™ Assays: Idylla™ ctKRAS, ctEGFR and ctNRAS-BRAF-EGFR S492R Mutation Assays (RUOs)



CONTACT US




Biocartis US Inc.
2 Pierce Place, Suite 1510
Itasca, IL 60143 - US
+1 (844) 443-9552

REQUEST A DEMO



Follow us on   
biocartis.com/us
customerserviceUS@biocartis.com



Idylla™ Platform is listed as a class II device in the US under establishment registration 3009972873. Idylla™ MSI Test (A0160/6) is cleared in the US under K211181 for Lynch Syndrome. Idylla™ CDx MSI Test (A0220/6) is approved in the US under P250005. Idylla™ EGFR, ctEGFR, BRAF, KRAS, ctKRAS, NRAS-BRAF-EGFR S492R, ctNRAS-BRAF-EGFR S492R, POLE-POLD1 & PIK3CA-AKT1 Mutation Assays; Idylla™ GeneFusion Assay; and Idylla™ IDH1-2 Mutation Assay Kit are for Research Use Only, not for use in diagnostic procedures. For more information on the acceptable use and licenses of Idylla™ products, please visit www.biocartis.com/en/license-statements. Biocartis and Idylla™ are registered trademarks in Europe, the US and many other countries. The Biocartis and Idylla™ trademarks and logos are used trademarks owned by Biocartis NV. Idylla™ is available for sale in Europe, the US and many other countries. Please check availability with a Biocartis representative.

© November 2025, Biocartis NV. All rights reserved.